


Supplementary figure S1. The calBP range vs radiocarbon determination from 101 BP to 5,100 BP. The areas denote the $\leq 0.1\%$, $\leq 0.2\%$, $\leq 0.3\%$, $\leq 0.4\%$, $\leq 0.5\%$, measurement precision for modern samples, as described in the text.

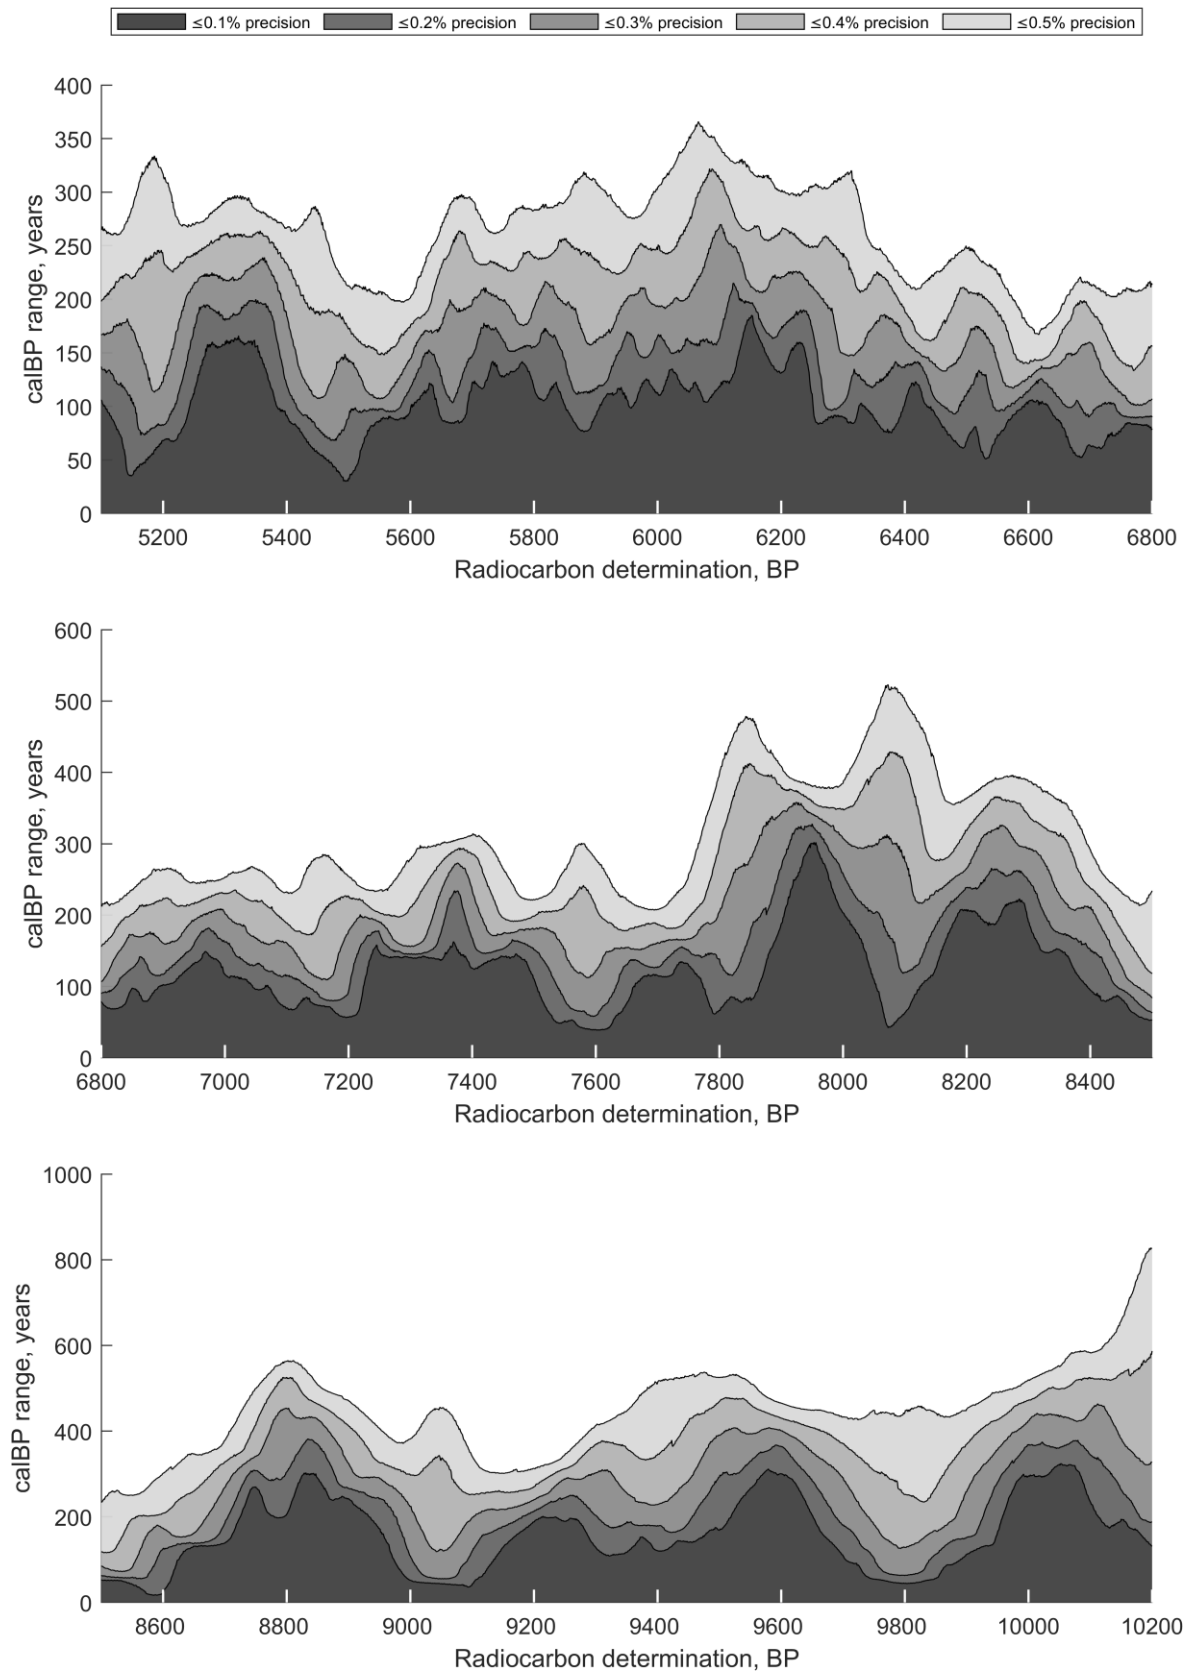

Supplementary figure S2. The calBP range vs radiocarbon determination from 5,100 BP to 10,200 BP. The areas denote the $\leq 0.1\%$, $\leq 0.2\%$, $\leq 0.3\%$, $\leq 0.4\%$, $\leq 0.5\%$, measurement precision for modern samples, as described in the text.